

# Embedded Fuzzy Classifier for Detection and Classification of Preseizure State Using Real EEG Data

Uvais Qidwai<sup>1</sup>, Aamir Saeed Malik<sup>2</sup>, and Mohamed Shakir<sup>2</sup>

<sup>1</sup>Computer Engineering Department, Qatar University, Qatar

<sup>2</sup>Neuro-Signal Processing Group, Centre for Intelligent Signal and Imaging Research

Universiti Teknologi PETRONAS, Tronoh, Perak

**Abstract**— A Classification technique using Fuzzy Logic Inference System to identify and predict the partial seizure from the epileptic EEG data along with preliminary brain conditions in different scenarios is presented in this paper. This detection system can produce warning signals for epileptic seizures. Electroencephalography (EEG) plays an important role, especially EEG based health diagnosis of brain disorder. However, the common clinical methods are insufficient when it comes to design an automated module to detect and predict partial seizure for epileptic patients. If the detection system is to be designed for ubiquitous applications, the system becomes even more complex if the patient is not confined to clinical environment when the device is monitoring continuously while the patient is involved in daily activities. Therefore, the work presented here includes embedded hardware system that works with classification algorithm on real EEG signals, in a ubiquitous setting. The performance of the system is shown under various conditions of daily activities. In order to make all this in a ubiquitous form factor, the algorithm for classification and detection of the pre-seizure conditions should be tremendously simple for processing the signal in a low cost ubiquitous microcontroller. This has been achieved in this work through the use of Fuzzy Classifiers based on the lookup table to empower system simplicity. The algorithm also utilizes certain statistical features from the EEG signal that are used as features to the classifier logic. While the clinical testing of the device is still awaited, various scenarios have been implemented using a custom-built hardware simulator based on empirical modeling of the real EEG signals. This shown various performance modes of the system and confirms the detection of pre-seizure state for a number of parameters related to the patients such as age, gender, etc... By using this type of fuzzy logic classifier, we were able to get over 90% accurate classifications for the partial seizure.

**Index Terms**— Fuzzy Classifier, Partial Seizure, Wearable Devices, Electroencephalography (EEG), Ubiquitous computing, Brain Computer Interface(BCI).

## I. INTRODUCTION

The EEG Embedded bio-signal Fuzzy Classifier is proposed for deploying disorder detection algorithms and signal processing in a portable system [1], by utilizing the power of LabVIEW for testing and to implement it into an embedded Data Acquisition System (DAQ). Patient module

can assess the signal and communicate the EEG data sets to a remote system for data processing and identification. Testing approach is obtained using the dataflow graphical form, with the combination of signal generation from the hardware for simulation of the Partial Pre-seizure EEG signal. This as a platform enables us to focus on the system design, system testing and rapid prototyping, even if lots of other languages for programming are accessible for constructing or generating the analog EEG signals and the specific part of the signal. In LabVIEW, basically the biomedical tool kit provides applications which are Ready-to-run. They in cooperate File Format Converter Player, Bio signal Data logger, Bio signal Generator, File Viewer, Blood Pressure (BP) Analyzer, Image Reconstruction of image in 3D, Feature Extractor for ECG, Variability Analyzer for the heartbeat rate. All the common file types' conversions are possible like the TDMS extension (National Instruments Technical Data Management Streaming), including ACQ, iWorx, Biopac, .edf, .mat, .txt and HL7. This tool kit is also capable of implementing algorithms for the signal processing on EEG bio signals. It also enables signal simulation of the signal, analysis of coherence and bi-spectral EEG, extraction of specific feature of the ECG, and power analysis of the EMG waveform, predefined virtual simulators for electroencephalography (EEG) and electrocardiogram (ECG). This system helps for the system which can be implemented and for the investigations of tiny, one-channel electroencephalogram systems in an ambulatory setting [2]. We will be using a part of this tool kit only just to validate the LabVIEW program build specifically to test the program data flow and its functionality to generate the pre-seizure signal from the real patient database via a DAQ and to transmit to a in range UN032 microcontroller from Digilent. This microcontroller reads the analog data from the inline analog to digital convertor port.

## II. METHOD AND DESIGN

For embedding algorithms in embedded platforms with low power consumptions, with computational constrains

and memory limitations [3], graphical FPGA design software play an important role in optimization. First, a dedicated system for this intension is built to improve with respect to the current system limitations, associated to approach of substantial processing, real-time healthcare facility accessibility and proper analysis. In the EEG DAQ simulator, the peak positions are not invariable, but may change from one region to another [4] from patient to patient. Here the procedure to simulate the EEG signal in LabVIEW environment and to detect the presence of healthy EEG and Pre-seizure signal which is to be detected by the cost effective microcontroller is achieved. The selection of EEG zones is simulated with respect to the alarm priority and two states which are also selected for the testing and execution in the initial prototype of the whole system. The LabVIEW program is used to simulate the abnormal EEG morphology [5], in three steps: (i) read the existing files recordings from a database or from the patient in real-time which may or may not contain normal, pre-seizure and seizure signals and (ii) simulate and transmit the EEG signal wired or wirelessly to the microcontroller (iii) the microcontroller will do all the fuzzy computation and generate a notification/alarm when pre-seizure signal is detected by using the algorithm.



Fig. 1. Functional System

In Figure 1, the system demonstrates a general setup for the experimentation and functioning flow. Here, the EEG signal waveform is fed from the LabVIEW to a NI-DAQ, which is available from commercially or for freely available data base which contains normal, pre-seizure and seizure datasets. Any irregular pattern in the data, then it prompts that an abnormal activity is present in the EEG [6] which could be seizure; and the program should be set to activate an alarm with respect to a set point in the program.

### III. EXPERIMENTAL SETUP

The simulation of real patient data in real time is obtained using NI X Series or NI-USB from National Instruments, which is a USB compatible device for acquisition and generation of data signals. This multifunctional device have

high performance digital I/O, control channels, counter/timers and analog measurement onto the portable wired or a wireless microcontroller (UNO32 in this test bench case). One disadvantage with this DAQ is that if we want to record and analyze more than 4 channels of EEG signals of the real time patients, then we have to use Analog-Digital MUX. So an additional 16 channels can be added.

In the subset of the program, the abnormal EEG dataset indicates central nervous system abnormality [7], cognitive states such as alertness and arousal [8]. This system also have the option to acquire in real time via EEG headsets like 128 channel headset or 16 channel head set like the Emotiv, and then transmit to the microcontroller for validation of the algorithm developed in order to identify by classification the state of pre-seizure in order to eliminate false prediction as much as possible. Once the algorithms have identified the pre-seizure, immediately the alarm is invoked in order to take precautionary acts to save the patient/user from more injury or accidents. By using a simulator we can optimize the electrode position in the patient when it comes to implementation of standalone microcontroller system to sense the EEG signal directly from the patient. The lesser number of ADCs input to the microcontroller, the faster the response to invoke the alarm. This also helps in simplify the computational algorithms, moreover frees temporary memory inside the microcontroller. The data from the DAQ is transferred to the microcontroller from the analog output port A01 of the USB-6008 DAQ. The microcontroller used in this setup is the mainboard ChipKIT UNO32.

In mode one (to simulate and experiment external EEG database), the EEG signal with pre-seizure and seizure patients, into the hardware DAQ, the EEG scalp data is used from CHB-MIT database. This EEG depository consists of dataset of twenty three patients (129 datasets with more than one seizure in .edf file format). The database of the EEG signal is provided by Boston children-hospital. The signals are sampled at the rate of 256 samples per second, with sixteen bits of resolution. Since the hardware simulator emulates the patient for the microcontroller, we can specifically select the channel to be transmitted to implement the algorithm on the individual channel to find out the individual response of the channel when processed by the microcontroller. In the microcontroller part, the statistical parameters like the energy, variance, kurtosis, Skewness etc. will be calculated on individual channel depending upon the user. This enables selectivity by the microcontroller.

IV. GENERATION OF EEG SIGNAL

The generation of signal from the EEG dataset is dependent of a number of variables [9]. This dataset changes from subject to subject and this simulator can generate any type of EEG signal. The seizure start points and end points have been clearly described in the database given by the CHB-MIT database. Before sending the test signal to the NI-DAQ hardware, the signal should be checked in the graph to select the start point of the seizure occurrence, manually by entering the values or parsing from a text file which contains an array of the file name, time (ms) and the waveform data. With respect to this, we calculate pre-seizure, seizure and normal EEG. We have arbitrary selected pre-seizure as ten seconds before the incidence of seizure, as per defined from the database. Twenty seconds before the seizure, is the start point of the normal EEG. Figure 2 shows a set of selected signals.

The ADC of the UNO32 microcontroller connected to the National Instruments DAQ ADC, the advantage is that it provides flexibility to the user to design our with EEG signal by using the Signal Simulator from the signal processing toolbox or toolkit. In this mode we can also create customized signal equations with respect the approximation model of EEG signal and generate the signal in the LabVIEW user interface program.

Once the algorithm is finalized in the microcontroller by using the signals from the EEG simulator workbench, it can be replaced with the real patient EEG data probe in real time on the fly. In this mode of operation, the UNO32 microcontroller will pre-process the input EEG signal from the human subject and look for a pre-seizure state. After

analysis and classification, if a pre-seizure state occurs, the microcontroller will alert locally and with the Bluetooth link to the mobile device. In future, we can add additional connectivity to the hospital database to transfer the time stamp of the occurrence of seizure/pre-seizure, location of occurrence and the EEG signal waveform itself at that time. This will help the medical doctor to look into more details about the EEG characteristics of the signal and the subject itself for further analysis by heuristics data. This software and the hardware provide support for the education and research of electrophysiology [10].

V. PROPOSED ALGORITHM

The raw EEG data is taken from the data depository of each of the patient randomly; therefore we have each EEG data set from the 24 patient. The selected data sets are: chb01\_03.edf, chb02\_16+.edf, chb03\_04.edf, chb04\_05.edf, chb05\_17.edf, chb06\_13.edf, chb07\_13.edf, chb08\_02.edf, chb09\_19.edf, chb10\_30.edf, chb11\_92.edf, chb12\_11.edf, chb13\_59.edf, chb14\_04.edf, chb15\_17.edf, chb16\_10.edf, chb17a\_04.edf, chb18\_31.edf, chb19\_30.edf, chb20\_16.edf, chb21\_22.edf, chb22\_25.edf, chb23\_06.edf and chb24\_13.edf [11]. Here for all the selected patients, the first channel has been used in the initial stage with the data value of 10 seconds each. This is done in order to reduce the load on the embedded processor later on. In order to test our algorithm’s capability to clearly distinguish the signal even if the noise exists, will be one of the challenges for this paper. The main algorithm modules for classification are shown in Figure 3.

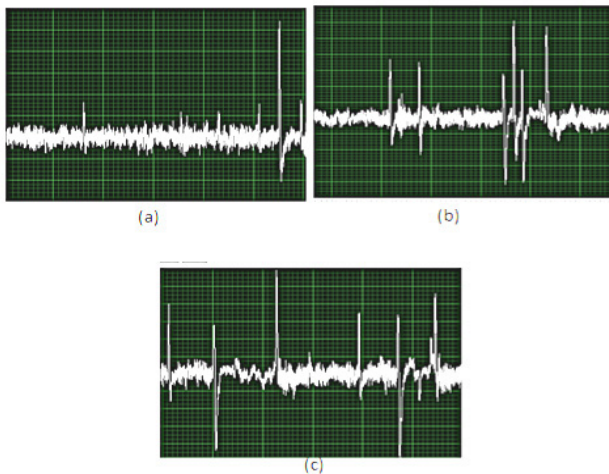


Fig. 2. Sample signal from the EEG data base in labVIEW graph: (a)Non-Seizure, (b) preseizure and ,(c) paritial Seizure.

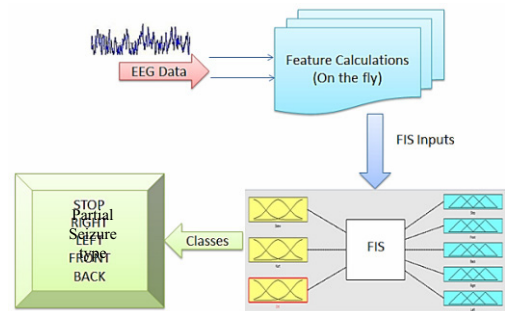


Fig. 3. Fuzzy Classification System.

As a preprocessing, we design a low pas filter, into which the raw data will be passed into. The signals which falls in channel 1 (FP1-F7) from the database is selected and then passed into Delta low pass FIR Filter , from 0Hz to 4 Hz of order 31. This will be ideal for a low cost microcontroller in consideration with low computation power. This is followed as a standard procedure for all the

24 patients’ iterations. This is done for the 10 seconds raw data window for normal, pre-seizure and seizure data set. Once the classification is solid, we have applied for the whole window of the raw data signal. This enables us to divide the signal into segments of frequency. This also enables us to suppress higher frequency components. Once the filtered signal is passed to the statistical tool box, we can make the classification possible for the Fuzzy Inference System.

VI. FUZZY INFERENCE SYSTEM

If we need to quantify perception of the human with respect to the ‘common sense’ information and its understanding by the perception of the surgeon, then Fuzzy Logic is the best tool for serving this purpose and to obtaining a better classification. The Matlab is used for Fuzzy system is obtained by using Fuzzy Logic Tool; Fuzzy Inference System (FIS) is developed with this bundle. Crisp values are not considered unlike the binary logic distinctions. When considering structure and its functionality, it is an innovative application for clinical data research; and also influential because it has the ability to interpret human expert heuristics as an input data of quantitative in nature to the system and consequently into useful estimates. The proposed FIS system consists of:

- two descriptors-membership as input (feature space representation as SF0 & SF1). Here SF0 represent the Variance , SF1 represents Entropy of the original signal.
- three descriptors-membership in lieu of cases and
- a set of 5 rules that represents the heuristical combination of the membership functions with historical understanding of the human user in the domain under study.

The membership function of the input, in which the grouping is individual, is represented in Figure 4(a)-(b). Initially, the EEG data obtained from the database were categorized into feature set of three. For these groups, we need to find the data class boundaries between them, for this purpose, we have applied C-Mean Fuzzy clustering. For each class (data set) of the input-membership these values of the boundary are used for formulating the system rule. In the fuzzy trapezoidal function, the boundary value shows the midpoint of every distribution of the membership. For better distinction, a gradient of 20% altogether is induced on either side. A mathematical map model can represent each degree, which will point to input value with respect to functional degree to have a fuzzified input data. Figure 10 shows output FIS variable, which indicates membership of

degree three reflecting the three status of the brain (normal, pre-seizure and seizure). Each of the memberships the triangular distributions is evenly distributed. These distributions are in degrees of: (a) ‘Un-likely’, (b) ‘Likely’, and (c) ‘Highly-likely’. For all the curves, the horizontal axis shows value of the input for every function of the membership and the vertical axis represents Boolean range (0-1) of the probability. Figure 5 shows the Output membership function.

The Rule-Base for Decisions

Centered with respect to heuristics(visual), six ‘rule’ are developed by using degree of the membership and logic high or low (1-0) is performed for specific type of input bundle, which corresponds data linked from membership function a decision that is either normal, pre-seizure or seizure is generated in combination with other decision-rule. This is also followed for rest of them. This produces a final decision surface. This rule is further taken into consideration with the decision of the physicians’ heuristics and a logical ‘AND’ operation is performed for the final decision; here mathematical model or statistical decision boundary is not used by any of the rule. Table 1 lists these rules.

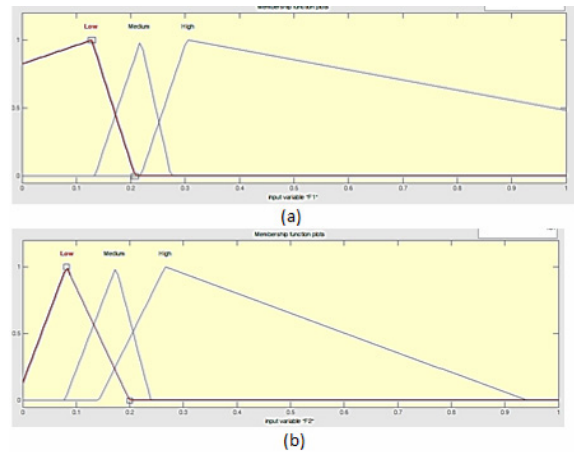


Fig. 4. Membership functions (Input); (a) SF0, (b) SF1.

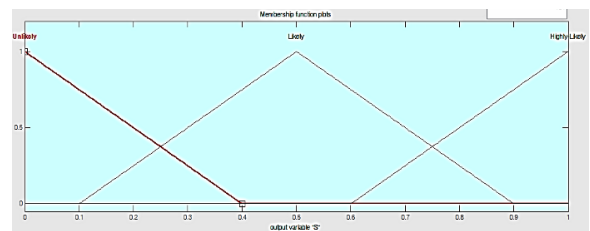


Fig. 5. Output Membership function.



Table 1: Rule- based on output for indication

Variance(SF0)	Entropy(SF1)	Output
High	High	Pre-Seizure
Low	Low	Seizure
High	Medium	Normal
Medium	High	Normal

The decision surface is calculated after the instructions based on the rule are designed. Here the centroid is obtained for the each group of input variables, which is then used where ever decision rule overlays with decision-surface for the input membership functions. Therefore the centroid is a significant value which indicates the degree where the inputs points to the rule-base. This ultimately provides a value that represents output degree. After the fuzzy classification is made, and when a clear differentiation is made, the data is passed from the laptop to the remote server or to a user mobile console for notification of the seizure disorders for monitoring and logging purpose.

VII. CONCLUSION

In this work, an approach is presented in order to modify an existing Data Acquisition/Generation module to function as an EEG simulator and to validate the identification of pre-seizure signal using statistical methods and fuzzy logic.

Such a system will be very helpful in EEG related research since all the initial algorithms can be tuned to the controlled data first before going to the actual human subjects. Unlike the commercial EEG simulators, to the best of our knowledge, there is no such commercially available system that can be used for such research tasks. The use of NI device and LabVIEW environment makes it very user friendly for anyone to develop a device tailored to their requirements. The data we have used is from actual patients and the system converts the text files for the data values into electrical voltages similar to what would be measured by the EEG probes. Further work is being done in producing more simulated data based on empirical models of the real waveforms. With controlled data types, Healthy/Normal, Seizure, and Pre-Seizure classes, the user can select the type and work on tuning their algorithms for detection and classification applications.

ACKNOWLEDGMENT

This publication was made possible by a grant from Qatar National Research Fund under its National Priority Research Program, for projects NPRP 09-292-2-113. Its contents are solely the responsibility of the authors and do not necessarily represent the official views of Qatar National Research Fund.

REFERENCES

- [1] Z. Khaliliardali, R. Chavarriaga, L. A. Gheorghe, and J. R. del Millan, "Detection of anticipatory brain potentials during car driving," *Engineering in Medicine and Biology Society (EMBC), 2012 Annual International Conference of the IEEE;* pp.3829,3832, Aug. 28 2012-Sept. 1 2012.
- [2] N. Katayama, K. Hidaka, A. Karashima, and M. Nakao, "Development of an immersive virtual reality system for mice," *SICE Annual Conference (SICE);* pp.791,794, 20-23 Aug. 2012.
- [3] A. Borgul, A. Margun, K. Zimenko, A. Kremlev, and A. Krasnov, "Intuitive control for robotic rehabilitation devices by human-machine interface with EMG and EEG signals," *Methods and Models in Automation and Robotics (MMAR);* pp.308,311, 27-30 Aug. 2012.
- [4] J. Duun-Henriksen, R. E. Madsen, L. S. Remvig, C. E. Thomsen, H. B. D. Sorensen, and T. W. Kjaer, "Automatic Detection of Childhood Absence Epilepsy Seizures: Toward a Monitoring Device," *Pediatric Neurology* ;Vol. 46, Issue 5, Pages 287-292, May 2012
- [5] S. Ravindran, and R. Cole, "Heart rate and epileptic seizure detection algorithms for low-power platforms," *Biomedical Signal Processing and Control*, Volume 7, Issue 3, May 2012.
- [6] Z. Ma, W. Zhou, Q. Yuan, and S. Geng, "Simulation of ictal EEG with a neuronal population model," *Bioelectronics and Bioinformatics (ISBB);* pp.103,106, 3-5 Nov. 2011.
- [7] W. Zhe, M. Hui, Ge. Manling, and G. Dong, "A Simulation of the Abnormal EEG Morphology by the 3-D Finite Element Method," *Engineering in Medicine and Biology Society, 2005. IEEE-EMBS.* pp.3620,3623, 17-18 Jan. 2006.
- [8] H. Meng; Z. Wang; M. Ge, X. Jiang, T. Zhang, J. Guo, and G. Dong, "An Understanding for the Abnormal Spikes of the EEG Simulation in a 2-D Neural Network," *Engineering in Medicine and Biology Society, 2005. IEEE-EMBS;*pp.3008,3011, Jan. 2006.
- [9] M. Ge, G. Dong, H. Meng, L. Wang, S. Yang, B. Wang, and C. Zhao, "An Abnormal EEG Simulation Based on The Chay Model of An Excitable Neuron," *Neural Engineering, 2005. Conference* ;pp.45,47, 16-19 March 2005
- [10] L. Rankine, H. Hassanpour, M. Mesbah, and B. Boashash, "Newborn EEG simulation from nonlinear analysis," *Signal Processing and Its Applications, 2005. Proceedings of the Eighth International Symposium* ; pp.191,194, August 28-31, 2005.
- [11] <http://www.emotiv.com/store/sdk/eeeg-bci/research-edition-sdk/>